

AmoyDx[®] HANDLE Classic NGS Panel

Instructions for Use

REF 8.06.0020

24 tests/kit

For Illumina MiSeqDx, NextSeq 550Dx



EC

REP

Amoy Diagnostics Co., Ltd. No. 39, Dingshan Road, Haicang District, 361027 Xiamen, P. R. China Tel: +86 592 6806835 Fax: +86 592 6806839 E-mail: sales@amoydx.com Website:www.amoydx.com Qarad EC-REP BV

Pas 257, 2440 Geel, Belgium

> Version: B1.1 Sept 2022



Background

Lung cancer is one of the most common malignant tumors, and 80-85% of lung cancers are non-small cell lung cancer (NSCLC). There are many driver mutations in NSCLC. The frequency of mutations in NSCLC for *EGFR*, *KRAS*, *NRAS*, *PIK3CA*, *BRAF*, *HER2* and *MET* gene are 10-35%, 5-30%, 1%, 3-5%, 1-4.9%, 2-4% and 1-5%, respectively. The frequency of gene fusion in NSCLC for *ALK*, *ROS1* and *RET* gene are 3-7%, 2% and 1-2% ^[1-8]. A large amount of clinical studies showed that gene mutation status is an important efficacy predictor for targeted therapy. For instance, *EGFR*-TKI would show better efficacy on patients with *EGFR* sensitizing mutation than wild-type gene ^[11]; the presence of the *ALK* and *ROS1* gene fusions is correlated with the efficacy of ALK/MET inhibitor therapy ^[2-3]; patients with *RET* fusion could benefit from MET/RET/VEGFR inhibitor^[4]; *BRAF* mutated patients will benefit from BRAF inhibitor treatment ^[5]; HER2 mutated patients will benefit from afatinib and the presence of KRAS, NRAS or PIK3CA gene mutation is correlated with primary resistance to EGFR-TKI ^[6-8]. It is indicated in NCCN Guideline for NSCLC that gene mutation testing is required before targeted therapy, and it is strongly recommended to conduct multi-target test for the optimal precision oncology treatment ^[9].

Colorectal cancer (CRC) is the third most common cancer worldwide with the metastatic disease accounts for 40-50% of newly diagnosed patients. In total, activating *KRAS*, *NRAS*, *PIK3CA* and *BRAF* mutations occur in 20-50%, 1-6%, 10-30% and 8-15% of colorectal cancers, respectively ^[10-11]. Clinical studies have shown that colorectal cancer patients with KRAS/NRAS/PIK3CA/BRAF mutation have poor response rate to anti-*EGFR* monoclonal antibodies ^[12-15]. Analysis of the mutation status of these four genes in patients with colorectal cancer helps to improve the objective response rate of the treatment.

With the development of genetic testing, especially the development of Next Generation Sequencing (NGS), more and more biomarkers have been discovered to develop better targeted therapy of pan cancer patients therapy. Recently, several TRK inhibitors have been proved to be very effective for various cancers, and patients with *NTRK1*, *NTRK2*, *NTRK3* rearrangements could benefit from TRK inhibitors ^[16-17]. There are also some very important biomarkers for pan cancer target therapy. Together with several important biomarkers guiding pan cancer target therapy, combined detection of multiple gene mutations in cancer patients is extremely important for effective precise treatment.

Please note that this kit has not been combined with drugs for clinical trials. It is only used for detection of common mutations in 40 genes listed in Table S1. The test results are for clinical reference only. Clinician should judge the test results based on the patient's condition, drug indications, treatment response and other laboratory test indicators comprehensively.

Intended Use

The AmoyDx[®] HANDLE Classic NGS Panel is a next-generation sequencing (NGS) based *in vitro* diagnostic assay intended for qualitative detection of single nucleotide variants (SNVs), insertions and deletions (InDels), gene fusions, copy number amplifications (CNAs) and microsatellite instability (MSI) in 40 key solid tumour genes (see Table S1 and S2), using DNA and RNA isolated from formalin-fixed paraffin embedded (FFPE) tumour tissue specimens. The assay is intended to provide tumor mutation profiling to be used by qualified health care professionals in accordance with professional guidelines in oncology for patients with solid malignant neoplasms.

This assay is not automated and is for laboratory professional use only.

Principles of the Procedure

The test kit is based on Halo-shape ANnealing and Defer-Ligation Enrichment system (HANDLE system) technology which is an improved Molecular Inversion Probe (MIP) technology to capture the target gene region (Figure 1). During the library construction process, each individual DNA molecule is tagged with a unique molecular index (UMI) at both ends, which allows high sensitivity in variant detection by eliminating any library amplification and sequencing bias.

The test kit uses both DNA and RNA extracted from FFPE samples, and it offers a time saving protocol that can be completed within 6 hours, and requires just about 1 hour of hands-on time. Firstly, the RNA is reverse transcribed into cDNA with help of the Reverse Transcriptase and the RT primers. Secondly, the cDNA product and the genomic DNA are combined together in one tube for hybridization. The probe contains an extension arm and a ligation arm which are complementary to the target gene region, and the probe anneals onto the DNA or cDNA template of the target region. Thirdly, the DNA is extended from the extension arm to the ligation arm with help of the DNA polymerase, then the nicks are repaired to generate the circular products with help of the DNA ligase. Next, the remaining linear probes, single-strand and double-strand DNA are digested with help of the exonuclease, and only the target circular DNA will be kept for PCR



amplification. Finally, the universal PCR amplification is performed to enrich the target libraries, and the magnetic bead-based purification is performed to obtain the final library.

After quality control (QC), the qualified libraries could be sequenced on Illumina sequencing platform. The sequencing data can be analyzed by AmoyDx NGS data analysis system (ANDAS) to detect the genomic variants in the target region.

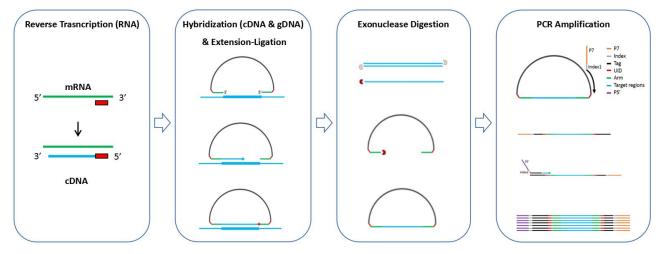


Figure 1 Principle of library construction (HANDLE system)

Kit Contents

This kit contains library construction reagents and positive controls (Table 1).

No.	Content	Main Ingredient	Quantity
1-RT	CP-RT Primers	Oligonucleotides	28 μL/tube × 1
2-RT	CP-RT Reaction Mix	Tris-HCl, K ⁺ , Mg ²⁺ , dNTPs,	$35 \mu\text{L/tube} \times 1$
3-RT	CP-Reverse Transcriptase	Reverse transcriptase	7 μL/tube × 1
4-Hyb	CP-Probe	Oligonucleotides	$28 \ \mu L/tube \times 1$
5-Hyb	CP-Hybridization Buffer	Tris-HCl, Mg ²⁺	28 μL/tube × 1
6-EL	CP-Extension Ligation Master Mix	DNA polymerase, dNTPs,DNA Ligase, Ligation buffer	28 μL/tube × 1
7-ED	CP-Exonuclease A	DNA Exonuclease	$14 \ \mu L/tube \times 1$
8-ED	CP-Exonuclease B	DNA Exonuclease	$14 \ \mu L/tube \times 1$
9-Amp	CP-PCR Master Mix	Tris, Mg ²⁺ , dNTPs, DNA polymerase	600 μL/tube × 1
502-522	CP-S5 Primer *	Oligonucleotides	5 μL/tube × 10
716-729	CP-N7 Primer *	Oligonucleotides	5 μL/tube × 12
PC-D	CP-Positive Control-DNA	DNA	$70 \ \mu L/tube \times 1$
PC-R	CP-Positive Control-RNA	RNA	70 μ L/tube × 1
NC-D	CP-Negative Control-DNA	DNA	$70 \ \mu L/tube \times 1$
NC-R	CP-Negative Control-RNA	RNA	70 μL/tube × 1

Table 1. Kit contents

* For labeling and sequence information of the primers, refer to Appendix Table S3.

Storage and Stability

The kit requires shipment on frozen ice packs and the shipping time should be less than one week. All contents of the kit should be stored immediately upon receipt at $-20\pm5^{\circ}$ C.

The shelf-life of the kit is twelve months. The recommended maximum freeze-thaw cycle is five cycles.

Additional Reagents and Equipment Required but Not Supplied

1) PCR instrument: Applied Biosystems[™] 2720 Thermal Cycler or MiniAmp[™] Thermal Cycler is recommended.



- 2) DNA quantification kit: QuantiFluor dsDNA System (Promega) or Qubit® dsDNA HS Assay Kit (Thermo Fisher Scientific) is recommended.
- 3) RNA quantification kit: QuantiFluor RNA System (Promega) or Qubit® RNA HS Assay Kit (Thermo Fisher Scientific) is recommended.
- 4) Fluorometer: Quantus™ Fluorometer (Promega), or Qubit 2.0/3/4 Fluorometer (Thermo Fisher Scientific) is recommended.
- 5) DNA/RNA extraction kit: AmoyDx[®] FFPE DNA/RNA Kit (AmoyDx) or AllPrep DNA/RNA FFPE Kit (Qiagen) is recommended for DNA and RNA co-extraction from FFPE sample. It is recommended to use RNase A (Thermo Fisher Scientific) to degrade RNA during the DNA extraction.
- 6) DNA purification kit: Agencourt AMPure XP Kit (Beckman Coulter) is recommended.
- 7) Sequencing reagent: Illumina 300 cycles (Paired-End Reads, 2×150 cycles) related reagents is recommended.
- 8) Sequencing instrument: Illumina MiSeqDx/NextSeq 550Dx is recommended.
- 9) Illumina PhiX Control V3.
- 10) Capillary electrophoresis analyzer and related kit: Agilent 2100 Bioanalyzer system and Agilent DNA 1000 Reagents (Agilent Technologies) or Agilent High Sensitivity DNA Kit (Agilent Technologies), or E-GelTM Power Snap Electrophoresis System (Thermo Fisher Scientific) and E-GelTM EX Agarose Gels, 2% (Thermo Fisher Scientific) is recommended.
- Magnetic Stand: DynaMag[™]-2 Magnet (Thermo Fisher Scientific) or DynaMag[™]-96 Side Magnet (Thermo Fisher Scientific) is recommended.
- 12) Vortex mixer.
- 13) Mini centrifuge.
- 14) Nuclease-free centrifuge tubes.
- 15) Nuclease-free PCR tubes.
- 16) Nuclease-free filtered pipette tips.
- 17) PCR-grade water (nuclease-free)
- 18) TE-low solution (10 mM Tris, 0.1 mM EDTA, pH 8.0) or 10 mM Tris (pH 8.0).
- 19) Ethanol (AR).
- 20) Ice box for 0.2 mL and 1.5 mL tubes.

Precautions and Handling Requirements

For in vitro diagnostic use

Precautions

- Please read the instruction carefully and become familiar with all components of the kit prior to use, and strictly follow the instruction during operation.
- Please check the compatible PCR instruments prior to use.
- DO NOT use the kit or any kit component after the expiry date.
- DO NOT use any other reagents from different lots.
- DO NOT use any other reagents from other test kits.

Safety Information

- Handle all specimens and components of the kit as potentially infectious material using safe laboratory procedures.
- Only trained professionals can use this kit. Please wear suitable lab coat and disposable gloves while handling the reagents.
- Avoid skin, eyes and mucous membranes contact with the chemicals. In case of contact, flush with water immediately.
- DO NOT pipette by mouth.

Decontamination and Disposal

- The kit contains positive control; strictly distinguish the positive control from other reagents to avoid contamination which may cause false positive.
- PCR amplification is extremely sensitive to cross-contamination. The flow of tubes, racks, pipets and other materials used should be



from pre-amplification to post-amplification, and never backwards.

- Gloves should be worn and changed frequently when handling samples and reagents to prevent contamination.
- Use separate, dedicated pipettes and filtered pipette tips when handling samples and reagents to prevent exogenous nucleic acid contamination to the reagents.
- All disposable materials are for one-time use. DO NOT reuse.
- The unused reagents, used reagents, and waste must be disposed properly.

Cleaning

• After the experiment, wipe down the work area, spray the pipettes and equipment with 75% ethanol or 10% hypochlorous acid solution.

Specimen Preparation

- Sample DNA and RNA should be extracted from FFPE tissue sample. The DNA will be used for the detection of SNV, InDel, CNA and MSI, and the RNA will be used for the detection of gene fusion and MET exon14 skipping.
- The FFPE tissue sample should be fixed by 10% neutral buffered formalin for 6~24 hours (no more than 24 hours). The freshly cut sections of FFPE tissue should be used for DNA extraction immediately. The storage time for the FFPE tissue should be less than 2 years.
- It is recommended that the tumor cell content is no less than 20%. For MSI and CNA detection, the recommended tumor cell content is no less than 30%.
- For surgical tumor resection specimens, it is recommended to use 2~6 unstained slides (5~10µM thick) for DNA/RNA extraction. For tissue biopsy specimens, it is recommended to use 10~15 unstained slides (5µM thick) for DNA/RNA extraction.
- It is recommended to use a commercialized DNA/RNA co-extraction kit to perform the DNA and RNA extraction, and use RNase A to degrade RNA during the DNA extraction. After extraction, measure the concentration of extracted DNA and RNA using Quantus[™] or Qubit[®]. The DNA concentration should be more than 6.25 ng/µL, and the total DNA should be more than 50 ng. The RNA concentration should be more than 4 ng/µL, and the total RNA should be more than 30 ng. For unqualified samples, re-collection or re-extraction are required.
- The qualified DNA and RNA should be used for library preparation immediately, if not, the DNA should be stored at -20 ± 5 °C and the RNA should be stored at -80 ± 5 °C for no more than 12 months, avoid repeated freezing and thawing.

Assay Procedure

Note:

- It is recommended to include a Positive Control (PC, DNA concentration is 6.25 ng/μL, RNA concentration is 4 ng/μL) and a Negative Control (NC, DNA concentration is 6.25 ng/μL, RNA concentration is 4 ng/μL) in the process of library construction, sequencing, and data analysis.
- During the following DNA library preparation process, please use the corresponding adaptor in the PCR instrument to avoid PCR product evaporation.
- It is recommended to use fluorescent dye method (Qubit or Quantus Fluorometer) for all the DNA/RNA concentration measurement step.

1. Reverse Transcription

- 1.1. Take out the (1-RT) **CP-RT Primers** and thaw the reagents at room temperature. When the reagents are completely thawed, mix well on a vortex mixer and centrifuge briefly, then keep the tube on ice.
- 1.2. Assemble the pre-reverse transcription reaction on ice in a nuclease-free 0.2mL PCR tube by adding the following components according to Table 2.

Reagent	Volume
Nuclease-free water	7.5-χ μL
RNA	χ μL
(1-RT) CP-RT Primers	1 µL
Total	8.5 μL

Table 2. Pre-reverse	transcription	reaction
----------------------	---------------	----------



Note:

- For FFPE samples, " χ " stands for the volume of 30~400 ng RNA (400 ng is recommended).
- For PC/NC RNA, χ=7.5 μL, take 7.5 μL (PC-R) CP-Positive Control-RNA / (NC-R) CP-Negative Control-RNA to construct library.
- 1.3. Mix the solution thoroughly by vortexing or pipetting, and centrifuge briefly, then place the sample in a thermocycler, set the reaction volume as 9 μL and perform the following program: <u>65°C for 5 min, then immediately transfer the tubes to ice for at least 1 min. Then proceed immediately to step 1.4.</u>
- 1.4. Take out the (2-RT) CP-RT Reaction Mix and thaw the reagents at room temperature. When the reagents are completely thawed, mix well on a vortex mixer and centrifuge briefly, then keep the tube on ice. Take out the CP-Reverse Transcriptase, mix well on a vortex mixer and centrifuge briefly, then keep the tube on ice. Assemble the reverse transcription reaction on ice by adding the following components according to Table 3.

Volume
1.25 μL
0.25 μL
8.5 μL
10 µL

Note: It is recommended to prepare freshly ready-to-use premix of CP-RT Reaction Mix and CP-Reverse Transcriptase for precise pipetting when perform three or more samples simultaneously.

1.5. Mix the solution thoroughly by vortexing or pipetting, and centrifuge briefly, then place the sample in a thermocycler, set the reaction volume as 10 μL and perform the following program: 50°C for 50 min, 98°C for 10 min, 4°C hold.

Note: The reverse transcription products should be stored at 2~8°C for no more than 20 hours if not proceed to the next step.

2. Hybridization

- 2.1. Take out the (4-Hyb) **CP-Probe** and (5-Hyb) **CP-Hybridization Buffer** and thaw the reagents at room temperature. When the reagents are completely thawed, mix well on a vortex mixer and centrifuge briefly, then keep the tube on ice.
- 2.2. Assemble the hybridization reaction on ice by adding the following components according to Table 4.

Reagent	Volume
Nuclease-free water	8-χ μL
DNA	χ μL
(4-Hyb) CP-Probe	1 µL
(5-Hyb) CP-Hybridization Buffer	1 µL
Reverse transcription product (from step 1.5)	10 µL
Total	20 µL

Note:

- For FFPE samples, " χ " stands for the volume of 50~100 ng DNA (70 ng is recommended).
- For PC/NC DNA, χ=8 μL, take 8 μL (PC-D) CP-Positive Control-DNA / (NC-D) CP-Negative Control-DNA to construct library.
- It is recommended to prepare *freshly ready-to-use premix* of CP-Probe and CP-Hybridization Buffer for precise pipetting when perform three or more samples simultaneously.
- 2.3. Mix the solution thoroughly by vortexing or pipetting, and centrifuge briefly, then place the sample in a thermocycler, set the reaction volume as 20 μL and perform the following program: <u>98°C for 5 min, 60°C for 2 h, 4°C hold.</u>
 Note: The hybridization products should be stored at 2~8°C for no more than 20 hours if not proceed to the next step.

3. Extension-Ligation

3.1. Take out the (6-EL) **CP-Extension Ligation Master Mix** and thaw the reagent at room temperature. When the reagents are completely thawed, mix well on a vortex mixer and centrifuge briefly, then keep the tube on ice.



3.2. Take out the above hybridization product from the thermocycler and keep the tube on ice. Add 1 μL (6-EL) CP-Extension Ligation Master Mix into the PCR tubes, mix the solution thoroughly by vortexing or pipetting, and centrifuge briefly, then place the sample in a thermocycler, set the reaction volume as 21 μL and perform the following program: <u>60°C for 10 min, 4°C hold.</u> Then proceed directly to the exonuclease digestion.

Note:

- Keep the tubes at low temperature after extension-ligation is finished, as high temperature like room temperature may increase the non-specificity. It is recommended to place the ice box besides the thermocycler, and when the extension-ligation program is finished, immediately transfer the tube on ice box.
- Perform the subsequent exonuclease digestion step immediately when the extension-ligation step is finished.

4. Exonuclease Digestion

- 4.1. Take out the (7-ED) **CP-Exonuclease A** and (8-ED) **CP-Exonuclease B**, mix well on a vortex mixer and centrifuge briefly, then keep the tube on ice.
- 4.2. Assemble the exonuclease digestion reaction on ice by adding the following components according to Table 5.

Reagent	Volume
(7-ED) CP-Exonuclease A	0.5 μL
(8-ED) CP-Exonuclease B	0.5 μL
Extension-Ligation product (from step 3.2)	21 µL
Total	22 μL

4.3. Mix the solution thoroughly by vortexing or pipetting, and centrifuge briefly, then place the sample in a thermocycler, set the reaction volume as 22 μL and perform the following program: <u>37°C for 30 min, 95°C for 10 min, 4°C hold.</u>

Note:

- It is recommended to prepare *freshly ready-to-use premix* of CP-Exonuclease A and CP-Exonuclease B for precise pipetting when perform three or more samples simultaneously.
- The products of exonuclease digestion should be stored at 2~8°C for no more than 20 hours if not proceed to the next step.

5. PCR Amplification

- 5.1. Take out the **CP-S5 Primer**, **CP-N7 Primer** and (9-Amp) **CP-PCR Master Mix** and thaw the reagents at room temperature. When the reagents are completely thawed, mix well on a vortex mixer and centrifuge briefly, then keep the tube on ice.
- 5.2. Assemble the PCR amplification reaction on ice by adding the following components according to Table 6.

Reagent	Volume
(9-Amp) CP-PCR Master Mix	25 μL
CP-S5 Primer	1.5 μL
CP-N7 Primer	1.5 μL
Exonuclease digestion product (from step 4.3)	22 µL
Total	50 µL

Note:

- Each of the CP-S5 Primer or CP-N7 Primer has a different index sequence. Use different combination of CP-S5 Primer and CP-N7 Primer for each sample library. **Do not** use the same combination of index for two or more sample libraries in one sequencing run. The detailed information for the index sequence is shown in Appendix.
- Transfer the prepared tubes to the amplification room to perform PCR amplification and the following purification to avoid contamination.
- 5.3. Mix the solution in each PCR tube thoroughly by vortexing or pipetting, and centrifuge briefly, then place the sample in a thermocycler, set the reaction volume as 50 μ L, and then perform the following program according to Table 7.



Table 7. PCR program			
Temperature	Time	Cycles	
98°C	1 min	1	
98°C	20 s		
61°C	30 s	25	
72°C	20 s		
72°C	5 min	1	
4°C	∞	1	

Note: The PCR products should be stored at 2~8°C for no more than 20 hours if not proceed to the next step.

6. Purification

- 6.1. Take out the AMPure XP beads and equilibrate them to room temperature for 30 min, and vortex the bottle of the beads to resuspend any magnetic particles that may have settled.
- 6.2. Add **40 μL resuspended beads** and **40 μL PCR products** into 1.5 mL centrifuge tubes, mix thoroughly by vortexing or pipetting, then incubate the mixture at room temperature for 5 min.
- 6.3. Place the centrifuge tubes onto the magnetic stand for 3~5 min until the solution turns clear. Gently remove and discard the supernatant while the centrifuge tube is on the magnetic stand. Do not touch the beads with pipette tip.
- 6.4. Keep the tubes on the magnetic stand, add 200 μL of freshly prepared 80% ethanol to the tube while in the magnetic rack. Incubate at room temperature for at least 30 seconds, and then carefully remove and discard the supernatant.
- 6.5. Repeat step 6.4 once.
- 6.6. Briefly spin the tube, and put the tube back in the magnetic rack. Completely remove the residual ethanol, and air dry the beads for 2~3 min while the tube is on the magnetic stand with the lid open.

Note: Do not over-dry the beads. This may result in lower recovery of DNA target.

- 6.8. Remove the tube from the magnet. Elute DNA target from the beads by adding 30 μL TE-low solution or 10 mM Tris solution (not provided), mix thoroughly by vortexing or pipetting, and incubate for 3 min at room temperature.
- 6.9. Put the tube in the magnetic rack for 3~5 min until the solution turns clear. Without disturbing the bead pellet, transfer the supernatant into a clean 1.5 mL centrifuge tube to obtain the final library.

Note: The purified library should be stored at -20°C for no more than two weeks if not proceed directly to sequencing.

7. Library Quality Control (QC)

- 7.1. Library concentration QC: Quantify the library concentration by Quantus[™] or Qubit[®] Fluorometer, the DNA concentration should be more than 10ng/μL, while 5~10 ng/μL was considered as risky (there is a risk of unqualified QC after data analysis).
- 7.2. Library fragment QC: Assess the library quality on an Agilent Bioanalyzer DNA chip, the main peak size of the DNA fragment should be at 150~400 bp, as shown in Figure 2.

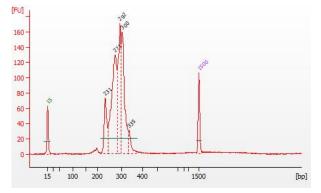


Figure 2. Example of library size distribution on a Bioanalyzer

AmoyDx ^{艾德生物}

Note:

- If the library QC pass, then move to sequencing. If not, the library should be reconstructed.
- If the library concentration is less than 5 ng/μL, the original DNA or RNA may be of poor quality or the DNA or RNA concentration may be inaccurate or there may be operational errors during the experiment. The DNA concentration should be retested, and it is recommended to input 100 ng DNA and perform overnight hybridization (60 °C for 12~18 h) to rebuild the library.

8. Sequencing

Illumina MiSeqDx or NextSeq 550Dx platform and corresponding Illumina 300 cycles (Paired-End Reads, 2×150 cycles) reagent is recommended for sequencing. The recommended percentage of Illumina PhiX Control v3 is 1%. The sequencing data per sample should be no less than 1 Gb and no more than 2 Gb when using NextSeq 550Dx platform, and no less than 375 Mb when using MiSeqDx platform. The suggested sample quantity per run is listed in Table 8.

Sequencing Instrument	Flow Cell	Read Length	Sample Quantity/Run
MiSeqDx	V3	2× 150 bp	20
NextSeq 550Dx	High	2× 150 bp	up to 120 [#]

Table 8. Recommended sequencing instruments and sample quantity per run

Maximum 120 indexes available. The PhiX percentage must be adjusted to ensure over-sequencing is not performed.

Perform the denaturation and dilution of the libraries according to the instrument's instructions. The final concentration of sequencing library is recommended in Table 9.

Table 9. Recommended final concentration of sequencing library

Sequencing Instrument	Final Concentration	
MiSeqDx	6~8 pM	
NextSeq 550Dx	0.6~1 pM	

Note: The concentration converting formula:

Library Concentration $[nM] = \frac{Library Concentration [ng/\mu L] \times 10^{6}}{660 \times 275}$

9. Data Analysis

When the sequencing is finished, adopt AmoyDx ANDAS Data Analyzer to analyze the sequencing data. Select the appropriate analysis module according to the sequencing platform, as shown in Table 10.

	2	
Sequencing Instrument	Data Throughput	Analysis Module
MiSeqDx	375 Mb/sample	ADXHS-Classic-M
NextSeq 550Dx	1 Gb/sample	ADXHS-Classic

Table 10. Analysis module

Check Q30 value for the sequencing data

If Q30 value of the sequencing data is ≥75%, the run data is qualified. If not, the sequencing data is unqualified.

Result Interpretation

The mutations are detected if meeting the following requirements.

- The "EffectiveDepth" of DNA should be no less than 400×, the "Depth" of each variant should be no less than 30×, and the inner RNA-Control should be no less than 20 copies.
- The filtering thresholds are listed in Table 11.



Sample Type	Parameter	ADXHS-Classic (NextSeq 550Dx)	ADXHS-Classic-M (MiSeqDx)
	Hot spot mutations of core regions (as shown in Table S4)	Freq \ge 0.5%, ADP \ge 4	Freq \geq 0.5%, ADP \geq 4
DNA	Hot spot mutations of non-core regions, non-hot spot mutations	Freq \ge 3%, ADP \ge 4	Freq \geq 3%, ADP \geq 4
	CNA	\geq 3.5 copy number	\geq 4 copy number
	MSINum	≥ 15%	≥ 15%
RNA	Fusions	≥ 10 copies	≥ 10 copies
	MET exon14 skipping	\geq 40 copies	\geq 40 copies

Table 11. Filtering thresholds

Note:

- Q30: one base call in 1,000 is predicted to be incorrect meaning a base call accuracy of 99.9%.
- *EffectiveDepth: The average depth of the target region after UMI calibration.*
- Depth: The effective depth of the variant site after UMI calibration.
- Freq: Frequency of mutant allele.
- *ADP: Depth of mutant allele.*
- MSINum: Percentage of microsatellite instability sites.
- The filtering thresholds in the ADXHS-Classic and ADXHS-Classic-M analysis modules are the same, while the effective depth calibration algorithm is different.
- For ADXHS-Classic-M analysis module, the detection of copy-number amplification (CNA) requires at least five samples to be extracted, library constructed, sequenced and analyzed simultaneously with reagents of the same lot. The CP-Positive Control and CP-Negative Control should be analyzed separately from the FFPE samples, otherwise it will affect the CNA detection of clinical samples.
- The PC should be detected as positive result for the corresponding mutation as shown in Table S5, and the NC should be detected as negative regarding the hotspot region. Otherwise, the Classic testing is unqualified, it is necessary to check if there is any operational error and the experiment should be repeated.
- If the RNA level test result is negative and the inner RNA-Control is less than 20 copies, it may be mainly due to poor RNA quality or insufficient amount of RNA input, or there may be some inhibitors in the RNA sample. It is recommended to re-extract RNA and reconstruct the library.
- If the detected MSINum value is between 12% and 26%, it is recommended to confirm the MSI status by PCR and capillary electrophoresis method.

Performances

1) Limit of Detection (LoD)

The LoD is listed in Table 12.

		1	
	Analysis Module	ADXHS-Classic (NextSeq 550Dx)	ADXHS-Classic-M (MiSeqDx)
	Hot spot mutations of core regions (Table S4)	Freq ≥ 1%	$Freq \ge 1\%$
DNA	Hot spot mutations of non-core regions, Non-hot spot mutations	$Freq \ge 5\%$	$Freq \ge 5\%$
	CNA	\geq 4 copy number	\geq 5 copy number
	MSI Tumor Purity	≥ 10%	≥ 10%
RNA –	Fusions	\geq 100 copies	\geq 200 copies
	MET exon14 skipping	\geq 250 copies	\geq 500 copies

Table 12. The LoD of Classic panel



3) Accuracy

Positive clinical FFPE specimens and positive reference standard were tested, and the positive percent agreement (PPA) for SNVs, Indels, fusions and CNAs detection was 100%, and the PPA for MSI detection was 96.9%.

4) Specificity

The negative percent agreement (NPA) for SNVs, Indels, fusions, CNAs and MSI detection was 100%.

5) Precision

Repeatability studies demonstrated 100% PPA and 100% NPA for all variants assessed across operators, instruments, and days.

Limitations

- 1) The kit is to be used only by personnel specially trained in the techniques of PCR and NGS.
- 2) The kit has been only validated for use with FFPE tissue samples.
- 3) Reliable results are dependent on proper sample processing, transport, and storage.
- 4) Negative results can not completely exclude the existence of mutated genes. Low tumor cell content, severe DNA/RNA degradation or the frequency under the limit of detection may also cause a false negative result.
- 5) Sampling of different sites of tumor tissue may lead to different test results due to tumor heterogeneity.
- 6) The test results of this kit are for clinical reference only and should not be used as the sole basis for individualized treatment of patients. Clinicians should make comprehensive judgments on the test results based on factors such as the patient's condition, drug indications, treatment response and other laboratory test indicators.
- 7) False negative results may occur when InDels occurs on the probe binding regions.
- The detection of MSI is only validated in FFPE samples from colorectal cancer and gastric cancer. MSI results from other cancers (eg. endometrial cancer, etc.) are for reference only.
- 9) The MSI status will be output as MSS or MSI. It does not distinguish between MSI-L and MSS.
- 10) Please strictly follow the sequence data volume recommended in the IFU, otherwise, it may lead to false negative or false positive results.

Reference

- 1. Reungwetwattana T, Dy GK. Targeted therapies in development for non-small cell lung cancer. J Carcinog. 2013, 12:22.
- 2. Gridelli C, Peters S, et al. ALK inhibitors in the treatment of advanced NSCLC. Cancer Treat Rev. 2014, 40(2):300-6.
- 3. Katayama R, Kobayashi Y, et al. Cabozantinib overcomes crizotinib resistance in ROS1 fusion-positive cancer. Clin Cancer Res. 2015, 21(1):166-74.
- 4. Drilon A, Wang L, et al. Response to Cabozantinib in Patients with RET Fusion-Positive Lung Adenocarcinomas. Cancer Discov. 2013, 3(6):630-5.
- Sánchez-Torres JM, Viteri S, et al. BRAF mutant non-small cell lung cancer and treatment with BRAF inhibitors. Transl Lung Cancer Res. 2013, 2(3):244-50.
- Califano R, Landi L, et al. Prognostic and predictive value of K-RAS mutations in non-small cell lung cancer. Drugs. 2012, 72 Suppl 1:28-36.
- 7. Stephens P, Hunter C, et al. Lung cancer: Intragenic ERBB2 kinase mutations in tumours. Nature. 2004, 431(7008):525–6.
- 8. Chen JY, Cheng YN, et al. Predictive value of K-ras and PIK3CA in non-small cell lung cancer patients treated with EGFR-TKIs: a systemic review and meta-analysis. Cancer Biol Med. 2015, 12(2):126–39.
- 9. NCCN Clinical Practice Guidelines in Oncology: Non-Small Cell Lung Cancer. Version 6. 2017.
- 10. http://www.nccn.org/professionals/physician_gls/f_guidelines.asp
- 11. Chan, E. 2015. Molecular Profiling of Colorectal Cancer. My Cancer Genome.
- 12. http://www.mycancergenome.org/content/disease/colorectal-cancer/ (Updated February 6).
- Douillard JY, Oliner KS, et al. Panitumumab-FOLFOX4 treatment and RAS mutations in colorectal cancer. N Engl J Med. 2013, 369(11):1023-34.
- 14. Di Bartolomeo M, Pietrantonio F, et al. Lack of KRAS, NRAS, BRAF and TP53 mutations improves outcome of elderly metastatic




colorectal cancer patients treated with cetuximab, oxaliplatin and UFT. Target Oncol. 2014, 9(2):155-62.

15. Heinemann V, von Weikersthal LF, et al. FOLFIRI plus cetuximab versus FOLFIRI plus bevacizumab as first-line treatment for patients with metastatic colorectal cancer (FIRE-3): a randomised, open-label, phase 3 trial. Lancet Oncol. 2014, 15(10):1065-75.

- 16. De Roock W, Claes B, et al. Effects of KRAS, BRAF, NRAS, and PIK3CA mutations on the efficacy of cetuximab plus chemotherapy in chemotherapy-refractory metastatic colorectal cancer: a retrospective consortium analysis. Lancet Oncol. 2010, 11(8):753-62.
- 17. National Comprehensive Cancer Network: NCCN Guidelines Colon Cancer (version 1.2015).
- 18. <u>http://www.nccn.org/professionals/physician_gls/f_guidelines.asp</u>
- 19. Drilon A. TRK inhibitors in TRK fusion-positive cancers. Ann Oncol. 2019 Nov 1;30(Suppl_8):viii23-viii30.
- 20. Wang Y, Long P, Wang Y, Ma W. NTRK Fusions and TRK Inhibitors: Potential Targeted Therapies for Adult Glioblastoma. Frontiers in Oncology. 2020 ;10:593578.

Symbols

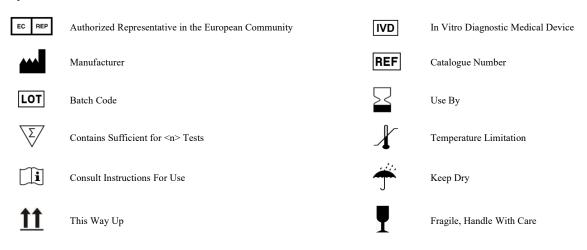

AmoyDx _{艾德生物}

Appendix

No.	Gene	Transcripts	Mutation	Related Exons
1	AKTI	NM_001014431	SNV, InDel	Exon 3,4
2	ALK	NM_004304	Fusion, SNV, InDel	Exon 21-25
3	BRAF	NM_004333	SNV, InDel	Exon 11,12,15,18
4	CDK4	NM_000075	CNA	/
5	CTNNB1	NM_001904	SNV, InDel	Exon 3
6	DDR2	NM_006182	SNV, InDel	Exon 5,8,13-18
7	DPYD*	NM_000110	SNPs	rs3918290, rs55886062, rs67376798, rs75017182
8	EGFR	NM_005228	SNV, InDel	Exon 3,7,12,14,18-22
9	ERBB2	NM_004448	SNV, InDel, CNA	Exon 1-27
10	ESR1	NM_001122740	SNV, InDel	Exon 6,9
11	FGFR1	NM_001174067	Fusion, SNV, InDel	Exon 5,6,13,15
12	FGFR2	NM_000141	Fusion, SNV, InDel	Exon 3,5-9,12-16,18
13	FGFR3	NM_000142	Fusion, SNV, InDel	Exon 3,7-15,17
14	FGFR4	NM_213647	SNV, InDel	Exon 3,6,9,10,12,13,15,16
15	HRAS	NM_001130442	SNV, InDel	Exon 2-4
16	IDH1	NM_005896	SNV, InDel	Exon 4
17	IDH2	NM_002168	SNV, InDel	Exon 4
18	KEAP1	NM_203500	SNV, InDel	Exon 2-6
19	KIT	NM_000222	SNV, InDel	Exon 9,11,13,14,17,18
20	KRAS	NM_033360	SNV, InDel	Exon 2-4
21	MAP2K1	NM_002755	SNV, InDel	Exon 2,3,6
22	MET	NM_000245	SNV, InDel, Exon14 Skipping, CNA	Exon 3,9,12,14,15,20,21
23	МҮС	NM_002467	CNA	/
24	NFE2L2	NM_006164	SNV, InDel	Exon 2
25	NKX2-1	NM_001079668	CNA	/
26	NRAS	NM_002524	SNV, InDel	Exon 2-4
27	NRG1	NM_013956	Fusion	/
28	NTRKI	NM_001007792	Fusion, SNV, InDel	Exon 14,15
29	NTRK2	NM_006180	Fusion, SNV, InDel	Exon 18,19
30	NTRK3	NM_002530	Fusion, SNV, InDel	Exon 16,17
31	PDGFRA	NM_006206	SNV, InDel	Exon 12,14,18
32	PIK3CA	NM_006218	SNV, InDel	Exon 2,3,5,6,8-10,14,21
33	POLE	NM_006231	SNV, InDel	Exon 3-14,19
34	PTEN	NM_000314	SNV, InDel	Whole CDS
35	RB1	NM_000321	SNV, InDel	Exon 1-27
36	RET	NM_020975	Fusion, SNV, InDel	Exon 5,6,8,10,11,13-16
37	ROSI	NM_002944	Fusion, SNV, InDel	Exon 36-38,40,41
38	STK11	NM_000455	SNV, InDel	Exon 1-9
39	TP53	NM_000546	SNV, InDel	Exon 2-11
40	UGT1A1*	NM_000463	SNPs	rs10929302, rs8175347, rs4148323
41	MSI	/	55 MSI Sites	/

Table S1. Target regions

Note: * The DPYD and UGT1A1 genes were covered to detect SNPs which are associated with cancer chemotherapy response.

AmoyDx _{艾德生物}

No.

54

No.	Fusions	Genes
1	BCL11A exon4-del15059ins14-ALK exon20	
2	BIRC6 exon10-ALK exon20	
3	CEBPZ exon2-ALK exon20	
4	CLIP1 exon22-ALK exon20	
5	COL25A1 exon3-ALK exon20	
6	DCTN1 exon26-ALK exon20	
7	EIF2AK3 exon2-ALK exon20	
8	EML4 exon13-ALK exon20	
9	EML4 exon13-ins69-ALK exon20	
10	EML4 exon14-del14-ALK exon20	
11	EML4 exon14-del38-ALK exon20	
12	EML4 exon14-del49ins11-ALK exon20	
13	EML4 exon15-del131-ALK exon20	
14	EML4 exon17-ALK exon20	
15	EML4 exon17-del46ins23-ALK exon20	
16	EML4 exon17-del46ins6-ALK exon20	
17	EML4 exon17-del58ins39-ALK exon20	1
18	EML4 exon17-ins30-ALK exon20	-
19	EML4 exon17-ins65-ALK exon20	
20	EML4 exon17-ins68-ALK exon20	-
21	EML4 exon17-ins95-ALK exon20	-
22	EML4 exon18-ALK exon20	-
23	EML4 exon20-ALK exon20	-
24	EML4 exon20-ins18-ALK exon20	_
25	EML4 exon2-ALK exon20	
26	EML4 exon2-ins117-ALK exon20	-
27	EML4 exon3-ins53-ALK exon20	-
28	EML4 exon6-ALK exon19	ALK
29	EML4 exon6-ALK exon20	-
30	EML4 exon6-ins18-ALK exon20	_
31	EML4 exon6-ins33-ALK exon20	_
32	GCC2 exon13-ALK exon20	_
33	GCC2 exon19-ALK exon20	_
34	HIP1 exon21-ALK exon20	_
35	HIP1 exon28-ALK exon20	-
36	HIP1 exon30-ALK exon20	_
37	KIF5B exon15-del14-ALK exon20	-
38	KIF5B exon17-ALK exon20	-
39	KIF5B exon24-ALK exon20	-
40	KLC1 exon9-ALK exon20	-
41	LMO7 exon15-ALK exon20	-
42	MPRIP exon21-ALK exon20	-
43	NBAS exon35-ALK exon20	-
44	PHACTR1 exon6-ALK exon20	-
45	PICALM exon19-ALK exon20	-
46	PPM1B exon1-ALK exon20	-
47	PRKAR1A exon10-ALK exon20	-
48	PRKAR1A exon5-ALK exon20	-
49	SQSTM1 exon5-ALK exon20	-
50	SUSTINI exon3-ALK exon20 STRN exon3-ALK exon20	-
50	TFG exon4-ALK exon20	-
52	TFG exon6-ALK exon20	-
53	TNIP2 exon5-ALK exon20	-
53	TDD amon 15 ALK amon 20	-

TPR exon15-ALK exon20

Fusions

57	CD74 exon6-ROS1 exon34	1
58	CD74 exon6-ROS1 exon35	1
59	CD74 exon8-ROS1 exon34	1
60	CLTC exon31-ROS1 exon35	1
61	EZR exon10-ROS1 exon34	1
62	EZR exon10-ROS1 exon35	1
63	GOPC exon4-ROS1 exon36	1
64	GOPC exon8-ROS1 exon35	-
65	KDELR2 exon5-ins8-ROS1 exon35	-
66	LRIG3 exon16-ROS1 exon35	-
67	MYO5A exon23-ROS1 exon35	ROSI
68	PPFIBP1 exon9-ROS1 exon35	
69	SDC4 exon2-ROS1 exon32	-
70	SDC4 exon4-ROS1 exon32	-
70	SDC4 exon4-ROS1 exon32	-
		-
72	SLC34A2 exon13-del47-ROS1 exon32	-
73	SLC34A2 exon13-del47-ROS1 exon34	-
74	SLC34A2 exon4-ROS1 exon32	-
75	SLC34A2 exon4-ROS1 exon34	-
76	TFG exon4-ROS1 exon35	4
77	TMEM106B exon3-ROS1 exon35	-
78	TPM3 exon7-ROS1 exon35	_
79	TPM3 exon8-ROS1 exon35	
80	AKAP13 exon35-RET exon12	
81	CCDC186 exon10-RET exon12	
82	CCDC186 exon7-RET exon12	
83	CCDC186 exon9-RET exon12	
84	CCDC6 exon1-del107-RET exon11	
85	CCDC6 exon1-del199-RET exon11	
86	CCDC6 exon1-ins132del125-RET exon11	1
87	CCDC6 exon1-RET exon10	1
88	CCDC6 exon1-RET exon12	1
89	CCDC6 exon1-RET exon2	1
90	CCDC6 exon2-RET exon11	-
91	CCDC6 exon2-RET exon12	-
92	CCDC6 exon8-RET exon12	-
93	CUX1 exon10-RET exon12	-
94	DLG5 exon13-RET exon12	RET
95	ERC1 exon10-RET exon12	
96	ERC1 exon12-RET exon12 ERC1 exon12-RET exon12	-
97	ERC1 exon12-RE1 exon12 ERC1 exon17-RET exon12	-
98	ERC1 exon7-RET exon12	-
		-
99	FKBP15 exon25-RET exon12	-
100	GOLGA5 exon7-RET exon12	-
101	HOOK3 exon11-RET exon12	-
102	RELCH exon10-RET exon12	4
103	KIF13A exon18-RET exon12	4
104	KIF5Bexon15-del107-RET exon11	4
105	KIF5B exon15-RET exon12	
106	KIF5B exon16-RET exon12	
107	KIF5B exon18-RET exon12	_
108	KIF5B exon22-RET exon12	

Fusions

CCDC6 exon5-ROS1 exon35

CD74 exon6-ROS1 exon32

Genes

Table S2. Gene fusions

No.

55

56

Genes



No.	Fusions	Genes	No.	Fusions	Genes
109	KIF5B exon23-RET exon12		164	FGFR2 exon17-DZANK1 exon11	
110	KIF5B exon24-RET exon11		165	FGFR2 exon17-EIF4A2 exon8	
111	KIF5B exon24-RET exon8		166	FGFR2 exon17-ERC1 exon7	
112	KTN1 exon29-RET exon12		167	FGFR2 exon17-GAB2 exon2	
113	MPRIP exon19-RET exon12		168	FGFR2 exon17-KIAA1217 exon3	
114	MYO5C exon25-RET exon12		169	FGFR2 exon17-SHTN1 exon7	
115	NCOA4 exon7-RET exon12		170	FGFR2 exon17-SHTN1 exon9	
116	NCOA4 exon8-del18-RET exon12		171	FGFR2 exon17-LZTFL1 exon8	
117	NCOA4 exon8-del199-RET exon11		172	FGFR2 exon17-OGA exon12	
118	NCOA4 exon8-RET exon12		173	FGFR2 exon17-NOL4 exon7	
119	NCOA4 exon9-RET exon12		174	FGFR2 exon17-NRAP exon24	
120	PCM1 exon29-RET exon12		175	FGFR2 exon17-NRBF2 exon4	
121	PICALM exon19-RET exon12	RET	176	FGFR2 exon17-OFD1 exon3	
122	PRKAR1A exon7-RET exon12		177	FGFR2 exon17-PAWR exon3	_
123	RUFY2 exon9-RET exon12		178	FGFR2 exon17-PCM1 exon7	_
124	RUFY3 exon12-RET exon12		179	FGFR2 exon17-POC1B exon11	
125	SPECC1L exon9-RET exon12		180	FGFR2 exon17-PPHLN1 exon3	-
126	TBL1XR1 exon9-RET exon12		181	FGFR2 exon17-PPP1R21 exon16	-
120	TNIP2 exon5-RET exon12		182	FGFR2 exon17-ROCK1 exon2	FGFR2
127	TRIM24 exon9-RET exon12	-	182	FGFR2 exon17-SEPTIN10 exon6	-
120	TRIM24 exon3-RET exon12	-	185	FGFR2 exon17-SLMAP exon2	-
130	TRIM27 exons-rel1 exon12 TRIM33 exon11-RET exon12	-	185	FGFR2 exon17-SORBS1 exon5	-
130	TRIM35 exon14-RET exon12		186	FGFR2 exon17-STK26 exon3	_
131	TRIM35 exon16-RET exon12		187	FGFR2 exon17-TACC2 exon11	
132	WAC exon3-RET exon12		187	FGFR2 exon17-TACC2 exon11	
133	FGFR1 exon18-TACC1 exon7		189	FGFR2 exon17-TACC5 exon11 FGFR2 exon17-TBC1D1 exon9	
					_
135	BAG4 exon1-FGFR1 exon3		190	FGFR2 exon17-TP73 exon2	_
136	BAG4 exon1-FGFR1 exon9	_	191	FGFR2 exon17-TXLNA exon5	
137	BAG4 exon2-FGFR1 exon7		192	FGFR2 exon17-WAC exon5	
138	ERLIN2 exon8-FGFR1 exon3		193	FGFR2 exon18-BICC1 exon2	
139	FN1 exon22-FGFR1 exon4	FGFR1	194	FGFR2 exon18-LAMC1 exon27	_
140	FN1 exon22-FGFR1 exon5		195	FGFR2 exon18-RABGAP1L exon20	
141	FN1 exon23-FGFR1 exon4		196	APIP exon1-FGFR2 exon10	
142	FN1 exon23-FGFR1 exon5		197	APIP exon1-FGFR2 exon6	
143	FN1 exon28-FGFR1 exon6		198	KLK2 exon1-FGFR2 exon5	
144	NSD3 exon1-FGFR1 exon3		199	SLC45A3 exon1-FGFR2 exon2	
145	FGFR2 exon17-AFF3 exon7		200	FGFR3 exon17-TLE5 exon2	_
146	FGFR2 exon17-AHCYL1 exon2		201	FGFR3 exon17-AMBRA1 exon16	_
147	FGFR2 exon17-AMOT exon3		202	FGFR3 exon17-BAIAP2L1 exon2	_
148	FGFR2 exon17-ATP6V1D exon3		203	FGFR3 exon17-del49-TACC3 exon4	_
149	FGFR2 exon17-BICC1 exon10		204	FGFR3 exon17-ELAVL3 exon2	_
150	FGFR2 exon17-BICC1 exon16		205	FGFR3 exon17-FBXO28 exon4	_
151	FGFR2 exon17-BICC1 exon18		206	FGFR3 exon17-JAKMIP1 exon4	
152	FGFR2 exon17-BICC1 exon2		207	FGFR3 exon17-PHLDB3 exon10	
153	FGFR2 exon17-BICC1 exon3		208	FGFR3 exon17-TACC3 exon10	
154	FGFR2 exon17-BICC1 exon9	FGFR2	209	FGFR3 exon17-TACC3 exon11	FGFR3
155	FGFR2 exon17-CASP7 exon3		210	FGFR3 exon17-TACC3 exon12	
156	FGFR2 exon17-CCAR2 exon4		211	FGFR3 exon17-TACC3 exon13	
157	FGFR2 exon17-CCDC186 exon4		212	FGFR3 exon17-TACC3 exon14	
158	FGFR2 exon17-CCDC6 exon2		213	FGFR3 exon17-TACC3 exon2	
159	FGFR2 exon17-CIT exon23		214	FGFR3 exon17-TACC3 exon3	
160	FGFR2 exon17-COL14A1 exon34		215	FGFR3 exon17-TACC3 exon6	
161	FGFR2 exon17-CREB5 exon8		216	FGFR3 exon17-TACC3 exon7	
162	FGFR2 exon17-CTNNA3 exon14		217	FGFR3 exon17-TACC3 exon8	
163	FGFR2 exon17-DDX21 exon2		218	FGFR3 exon18-del112-TACC3 exon10	\neg



No.	Fusions	Genes	No.	Fusions	Genes
219	FGFR3 exon18-del117-TACC3 exon8		274	ZMYM2 exon2-NRG1 exon2	NRG1
220	FGFR3 exon18-del124-TACC3 exon9		275	AFAP1 exon4-NTRK1 exon9	
221	FGFR3 exon18-del125-TACC3 exon11	FGFR3	276	AMOTL2 exon6-NTRK1 exon12	
222	FGFR3 exon18-del147-TACC3 exon7	FGFKS	277	ARHGEF2 exon21-NTRK1 exon10	
223	FGFR3 exon18-del27-TACC3 exon11		278	ATP1B1 exon2-NTRK1 exon8	
224	FGFR3 exon18-del37ins15-TACC3 exon9		279	ARHGEF11 exon40-NTRK1 exon12	
225	ADAM9 exon18-NRG1 exon2		280	BCAN exon12-NTRK1 exon10	
226	AKAP13 exon5-NRG1 exon2		281	BCAN exon13-NTRK1 exon11	
227	ATP1B1 exon2-NRG1 exon2		282	CD74 exon8-NTRK1 exon10	
228	CD44 exon5-NRG1 exon2	-	283	CD74 exon8-NTRK1 exon12	-
229	CD74 exon6-NRG1 exon3	_	284	CEL exon7-NTRK1 exon8	
230	CD74 exon6-NRG1 exon6	_	285	CHTOP exon5-NTRK1 exon10	-
231	CD74 exon7-NRG1 exon2	_	286	CHTOP exon5-NTRK1 exon11	-
232	CD74 exon7-NRG1 exon6	_	287	CTRC exon1-NTRK1 exon8	-
		_			_
233	CD74 exon8-NRG1 exon6	_	288	DIAPH1 exon26-NTRK1 exon10	-
234	CDH1 exon2-NRG1 exon2	_	289	EPHB2 exon3-NTRK1 exon8	_
235	CLU exon2-NRG1 exon6	4	290	EPS15 exon21-NTRK1 exon10	_
236	COX10-AS1 exon1-NRG1 exon2	4	291	F11 exon4-NTRK1 exon10	4
237	DIP2B exon1-NRG1 exon2	4	292	F11R exon4-NTRK1 exon10	_
238	DPYSL2 exon7-NRG1 exon6	4	293	GRIPAP1 exon22-NTRK1 exon10	_
239	GDF15 exon1-NRG1 exon2		294	GRIPAP1 exon22-NTRK1 exon11	_
240	HMBOX1 exon1-NRG1 exon6		295	GRIPAP1 exon22-NTRK1 exon12	
241	KIF13B exon2-NRG1 exon2		296	GON4L exon21-NTRK1 exon8	
242	MCPH1 exon10-NRG1 exon2		297	IRF2BP2 exon1-del48-NTRK1 exon10	
243	MDK exon4-NRG1 exon6		298	IRF2BP2 exon1-NTRK1 exon10	
244	MRPL13 exon2-NRG1 exon2		299	IRF2BP2 exon1-NTRK1 exon8	
245	MTSS1 exon3-NRG1 exon2		300	KIF21B exon14-NTRK1 exon10	
246	NOTCH2 exon4-NRG1 exon6		301	LMNA exon2-NTRK1 exon10	
247	PARP8 exon3-NRG1 exon2		302	LMNA exon4-NTRK1 exon10	NTRKI
248	PCM1 exon2-NRG1 exon6		303	LMNA exon9-NTRK1 exon10	
249	PDE7A exon3-NRG1 exon6	NRG1	304	LMNA exon9-NTRK1 exon12	
250	POMK exon2-NRG1 exon2		305	LMNA exon10-NTRK1 exon10	_
251	RAB3IL1 exon9-NRG1 exon6	_	306	LMNA exon10-NTRK1 exon11	
252	RALGAPA1 exon20-NRG1 exon6	_	307	LMNA exon10-NTRK1 exon12	_
252	RBPMS exon5-NRG1 exon2	-	308	LMNA exon11-NTRK1 exon12	_
255	RBPMS exon5-NRG1 exon6	_	309	LMNA exon11-del150-NTRK1 exon11	_
		_		LMNA exon12-NTRK1 exon12	
255	ROCK1 exon1-NRG1 exon2	-	310		-
256	SDC4 exon2-NRG1 exon4	-	311	LMNA exon2-NTRK1 exon11	4
257	SDC4 exon2-NRG1 exon6	4	312	LMNA exon2-NTRK1 exon12	-
258	SDC4 exon4-NRG1 exon6	4	313	LMNA exon2-NTRK1 exon16	_
259	SETD4 exon2-NRG1 exon2	4	314	LMNA exon3-NTRK1 exon11	4
260	SLC3A2 exon4-NRG1 exon6	_	315	LMNA exon4-NTRK1 exon12	4
261	SLC3A2 exon5-NRG1 exon6		316	LMNA exon5-NTRK1 exon11	
262	SLC4A4 exon14-NRG1 exon2		317	LMNA exon6-del172-NTRK1 exon12	_
263	SMAD4 exon1-NRG1 exon6		318	LMNA exon8-NTRK1 exon12	
264	TENM4 exon12-NRG1 exon2		319	LMNA UTR3-NTRK1 exon12	
265	THAP7 exon3-NRG1 exon2		320	LRRC71 exon1-NTRK1 exon10	
266	THBS1 exon6-NRG1 exon6		321	MEF2D exon9-NTRK1 exon12	
267	TNC exon10-NRG1 exon6		322	MPRIP exon14-NTRK1 exon12	
268	TNKS exon3-NRG1 exon2	1	323	MPRIP exon18-NTRK1 exon12	
269	TSHZ2 exon1-NRG1 exon6	-	324	MPRIP exon21-NTRK1 exon12	-
270	VAMP2 exon4-NRG1 exon4	-	325	MPRIP exon21-NTRK1 exon14	-
271	VTCN1 exon2-NRG1 exon4	-	326	MTMR6 exon1-NTRK1 exon8	-
272	NSD3 exon1-NRG1 exon2	-	327	NFASC exon20-NTRK1 exon10	-
	1.555 enour futor enous	1	527		1



No.	Fusions	Genes	No.	Fusions	Genes
329	PEAR1 exon15-NTRK1 exon10		384	QKI exon6-NTRK2 exon16	
330	PLEKHA6 exon14-NTRK1 exon10		385	SPECC1L exon10-NTRK2 exon15	
331	PLEKHA6 exon21-NTRK1 exon10		386	SPECC1L exon11-NTRK2 exon15	
332	PLEKHA6 exon21-NTRK1 exon9		387	SQSTM1 exon4-NTRK2 exon15	
333	PPL exon11-NTRK1 exon13		388	SQSTM1 exon5-NTRK2 exon16	
334	PPL exon21-NTRK1 exon10	-	389	SQSTM1 exon5-NTRK2 exon17	
335	PPL exon21-NTRK1 exon11	-	390	STRN exon3-NTRK2 exon16	
336	PPL exon22-del3058-NTRK1 exon11	-	391	STRN3 exon7-NTRK2 exon16	_
337	PRDX1 exon5-NTRK1 exon12	-	392	TBC1D2 exon6-NTRK2 exon14	NTRK2
338	RPL7A exon2-NTRK1 exon10	-	393	TLE4 exon7-NTRK2 exon15	-
339	SCYL3 exon11-NTRK1 exon12	-	394	TRAF2 exon9-NTRK2 exon15	-
340	SQSTM1 exon2-NTRK1 exon10	-	395	TRIM24 exon12-NTRK2 exon15	-
341	SQSTM1 exon5-NTRK1 exon10	-	396	TRIM24 exon12-NTRK2 exon16	-
342	SQSTM1 exon6-NTRK1 exon10	-	397	VCAN exon6-NTRK2 exon12	_
343	SSBP2 exon12-NTRK1 exon12	-	398	VCL exon16-NTRK2 exon12	_
343		-	398	WNK2 exon24-NTRK2 exon16	_
	TFG exon4-NTRK1 exon9				
345	TFG exon5-del258-NTRK1 exon8	_	400	AKAP13 exon3-NTRK3 exon14	_
346	TFG exon5-NTRK1 exon10	4	401	AKAP13 exon14-NTRK3 exon14	-
347	TFG exon5-NTRK1 exon9	_	402	AKAP13 exon16-NTRK3 exon14	_
348	TFG exon6-NTRK1 exon10	_	403	BTBD1 exon4-NTRK3 exon14	_
349	TNFSF15 exon1-NTRK1 exon11	NTRKI	404	EEF1A1 exon8-NTRK3 exon14	_
350	TPM3 exon1-del132-NTRK1 exon12	_	405	EML4 exon2-NTRK3 exon14	
351	TPM3 exon5-NTRK1 exon11		406	EML4 exon6-NTRK3 exon14	
352	TPM3 exon5-NTRK1 exon12		407	ETV6 exon4-NTRK3 exon12	
353	TPM3 exon7-NTRK1 exon10		408	ETV6 exon4-NTRK3 exon13	
354	TPM3 exon7-del39-NTRK1 exon10		409	ETV6 exon4-NTRK3 exon14	
355	TPM3 exon8-NTRK1 exon10		410	ETV6 exon4-NTRK3 exon15	
356	TPM3 exon8-NTRK1 exon12		411	ETV6 exon5-NTRK3 exon13	
357	TPM3 exon9-NTRK1 exon10		412	ETV6 exon5-NTRK3 exon14	
358	TPM3 exon10-NTRK1 exon8		413	ETV6 exon5-NTRK3 exon15	
359	TPM3 exon10-NTRK1 exon9		414	ETV6 exon5-NTRK3 exon16	
360	TPM3 UTR3-NTRK1 exon9		415	ETV6 exon6-NTRK3 exon13	
361	TPR exon10-NTRK1 exon10		416	ETV6 exon6-NTRK3 exon15	
362	TPR exon16-del54ins13-NTRK1 exon10		417	KANK1 exon2-NTRK3 exon14	
363	TPR exon21-NTRK1 exon10		418	LYN exon8-NTRK3 exon14	
364	TPR exon21-NTRK1 exon9		419	MYO5A exon23-NTRK3 exon11	NTRK3
365	TPR exon22-NTRK1 exon10		420	MYO5A exon23-NTRK3 exon12	
366	TPR exon6-NTRK1 exon12	-	421	MYO5A exon32-NTRK3 exon13	
367	TRIM33 exon12-NTRK1 exon12	-	422	PHACTR1 exon5-NTRK3 exon14	
368	TRIM63 exon8-NTRK1 exon9	-	423	PHACTR1 exon7-NTRK3 exon14	
369	VANGL2 exon1-NTRK1 exon12	-	424	RBPMS exon5-NTRK3 exon14	_
370	ZBTB7B exon4-NTRK1 exon12	-	425	SNHG26 exon3-NTRK3 exon16	-
371	AFAP1 exon13-NTRK2 exon12	+	426	SPECC1L exon5-NTRK3 exon14	-
372	AGBL4 exon5-NTRK2 exon16	-	427	SPECC1L exon8-NTRK3 exon13	-
372	AGBL4 exon6-NTRK2 exon16	-	427	SQSTM1 exon4-NTRK3 exon14	-
373	AGBL4 exon7-NTRK2 exon16	-	428	SQSTM1 exon5-NTRK3 exon14	-
		-	429	· · · · · · · · · · · · · · · · · · ·	-
375	BCR exon1-NTRK2 exon17	-		SQSTM1 exon6-NTRK3 exon15	-
376	ETV6 exon5-NTRK2 exon15	NTD V2	431	SQSTM1 exon7-NTRK3 exon14	-
377	GKAP1 exon9-NTRK2 exon16	NTRK2	432	STRN exon3-NTRK3 exon14	-
378	KANK1 exon11-NTRK2 exon14	4	433	STRN3 exon3-NTRK3 exon14	_
379	KCTD8 exon1-NTRK2 exon16	4	434	TFG exon6-NTRK3 exon14	_
380	NACC2 exon5-NTRK2 exon13	_	435	TMTC2 exon9-NTRK3 exon15	_
381	NOS1AP exon9-NTRK2 exon13		436	VIM exon8-NTRK3 exon14	_
382	PAN3 exon1-NTRK2 exon17	_	437	WDR72 exon18-NTRK3 exon15	
383	PRKAR2A exon2-NTRK2 exon16		/	/	/



Name	Primer Index Information	Illumina Nextera XT v2Set D No.
CP-N716	TAGCGAGT	N716
CP-N718	GTAGCTCC	N718
CP-N719	TACTACGC	N719
CP-N720	AGGCTCCG	N720
CP-N721	GCAGCGTA	N721
CP-N722	CTGCGCAT	N722
CP-N723	GAGCGCTA	N723
CP-N724	CGCTCAGT	N724
CP-N726	GTCTTAGG	N726
CP-N727	ACTGATCG	N727
CP-N728	TAGCTGCA	N728
CP-N729	GACGTCGA	N729
CP-S502	CTCTCTAT	\$502
CP-S503	TATCCTCT	S503
CP-S513	TCGACTAG	S513
CP-S515	TTCTAGCT	S515
CP-S516	CCTAGAGT	S516
CP-S517	GCGTAAGA	S517
CP-S518	CTATTAAG	S518
CP-S520	AAGGCTAT	\$520
CP-S521	GAGCCTTA	\$521
CP-S522	TTATGCGA	\$522

Table S3. Index sequence information for primers

Table S4. Core regions (sensitivity of 1%, tagged as VIP in the ANDAS output file)

No.	Gene	Core Regions	Representative Hot Spot Mutations
01	BRAF	NM_004333.4: exon15	V600E
02	EGFR	NM_005228.3: Exon18	G719S
03	EGFR	NM_005228.3: Exon19	E746_A750del
04	EGFR	NM_005228.3: Exon20	S768I、D770_N771insG、T790M
05	EGFR	NM_005228.3:Exon21	L858R、L861Q
06	ERBB2	NM_004448.3:Exon20	A775_G776insYVMA
07	KRAS	NM_033360.3:Exon2	G12C、G12S、G12D、G12V
08	KRAS	NM_033360.3:Exon3	Q61H
09	NRAS	NM_002524.4:Exon2	G12D
10	NRAS	NM_002524.4:Exon3	Q61K、Q61R
11	PIK3CA	NM_006218.2:Exon10	E545K
12	PIK3CA	NM_006218.2:Exon21	H1047R

Table S5. Hot spot mutations (tagged as VIP in the ANDAS output file) and fusions of CP-Positive Control (DNA&RNA)

No.	Gene	Mutation
01	EGFR	NM_005228.3:exon20:c.2369C>T:p.(T790M)
02	EGFR	NM_005228.3:exon21:c.2573T>G:p.(L858R)
03	EGFR	NM_005228.3:exon19:c.2235_2249del15:p.(E746_A750del)
04	KRAS	NM_033360.3:exon2:c.38G>A:p.(G13D)
05	PIK3CA	NM_006218.2:exon10:c.1633G>A:p.(E545K)
06	PIK3CA	NM_006218.2:exon10:c.1645G>A:p.(D549N)
07	ROS1	SLC34A2:NM_006424.2:exon4-ROS1:NM_002944.2:exon32
08	ROS1	SLC34A2:NM_006424.2:exon4-ROS1:NM_002944.2:exon34
09	/	MSI-H

Note: Please note that there is an additional positive variant in PC, PIK3CA Exon3: c.353G>A:p.(G118D), but this variant is not necessary for quality control. It will be detected under normal circumstances, but occasionally they may be missed.